

CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma)

Package Insert

REF	CK-MB	English
-----	-------	---------

A rapid test for the diagnosis of myocardial infarction (MI) to detect CK-MB qualitatively in whole blood, serum or plasma.

For professional *in vitro* diagnostic use only.

【INTENDED USE】

The CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma) is a rapid chromatographic immunoassay for the qualitative detection of human CK-MB in whole blood, serum or plasma as an aid in the diagnosis of myocardial infarction (MI).

【SUMMARY】

Creatine Kinase MB (CK-MB) is an enzyme present in the cardiac muscle with a molecular weight of 87.0 kDa.¹ Creatine Kinase is a dimeric molecule formed from two subunits designated as "M" and "B" which combine to form three different isoenzymes, CK-MM, CK-BB, and CK-MB. CK-MB is the isoenzyme of Creatine Kinase most involved in the metabolism of cardiac muscle tissue.²

The release of CK-MB into the blood following MI can be detected within 3-8 hours after the onset of symptoms. It peaks within 9 to 30 hours, and returns to baseline levels within 48 to 72 hours.³ CK-MB is one of the most important cardiac markers and is widely recognized as the traditional marker for the diagnosis of MI.

The CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma) is a simple test that utilizes a combination of antibody coated particles and capture reagents to qualitatively detect CK-MB in whole blood, serum or plasma. The minimum detection level is 5 ng/mL CK-MB.

【PRINCIPLE】

The CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma) is a qualitative, membrane based immunoassay for the detection of CK-MB in whole blood, serum or plasma. The membrane is pre-coated with specific capture antibodies in the test line regions of the test. During testing, the whole blood, serum or plasma specimen reacts with the particle coated with specific antibodies. The mixture migrates upward on the membrane chromatographically by capillary action to react with specific capture reagents on the membrane and generate a colored line. The presence of this colored line in the specific test line region indicates a positive result, while its absence indicates a negative result. To serve as a procedural control, a colored line will always appear in the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred.

【REAGENTS】

The test contains anti-CK-MB antibody conjugated colloid gold particles and capture reagents coated on the membrane.

【PRECAUTIONS】

- For professional *in vitro* diagnostic use only. Do not use after expiration date.
- Do not eat, drink or smoke in the area where the specimens or kits are handled.
- Do not use test if pouch is damaged.
- Handle all specimens as if they contain infectious agents. Observe established precautions against microbiological hazards throughout all procedures and follow the standard procedures for proper disposal of specimens.
- Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are assayed.
- The used test should be discarded according to local regulations.
- Humidity and temperature can adversely affect results.

【STORAGE AND STABILITY】

Store as packaged in the sealed pouch either at room temperature or refrigerated (2-30 °C). The test is stable through the expiration date printed on the sealed pouch. The test must remain in the sealed pouch until use. **DO NOT FREEZE.** Do not use after the expiration date.

【SPECIMEN COLLECTION AND PREPARATION】

- The CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma) can be performed using whole blood (from venipuncture or fingerstick), serum or plasma.
- To collect **Fingerstick Whole Blood specimens**:
 - Wash the patient's hand with soap and warm water or clean with an alcohol swab. Allow to dry.
 - Massage the hand without touching the puncture site by rubbing down the hand towards the fingertip of the middle or ring finger.
 - Puncture the skin with a sterile lancet. Wipe away the first sign of blood.
 - Gently rub the hand from wrist to palm to finger to form a rounded drop of blood over the puncture site.
- Add the Fingerstick Whole Blood specimen to the test by using **a capillary tube**:
 - Touch the end of the capillary tube to the blood until filled to approximately 75 μ L. Avoid air bubbles.
 - Place the bulb onto the top end of the capillary tube, then squeeze the bulb to dispense the whole blood to the specimen area of the test cassette.

- Add the Fingerstick Whole Blood specimen to the test by using **hanging drops**:
 - Position the patient's finger so that the drop of blood is just above the specimen well of the test cassette.
 - Allow 3 hanging drops of fingerstick whole blood to fall into the center of the specimen area on the test cassette, or move the patient's finger so that the hanging drop touches the center of the specimen well. Avoid touching the finger directly to the specimen area.
- Separate serum or plasma from blood as soon as possible to avoid hemolysis. Use only cleanon-hemolyzed specimens.
- Testing should be performed immediately after the specimens have been collected. Do not leave the specimens at room temperature for prolonged periods. Serum and plasma specimens may be stored at 2-8 °C for up to 3 days. For long term storage, specimens should be kept below -20 °C. Whole blood collected by venipuncture should be stored at 2-8 °C if the test is to be run within 2 days of collection. Do not freeze whole blood specimens. Whole blood collected by fingerstick should be tested immediately.
- Bring specimens to room temperature prior to testing. Frozen specimens must be completely thawed and mixed well prior to testing. Specimens should not be frozen and thawed repeatedly.
- If specimens are to be shipped, they should be packed in compliance with local regulations covering the transportation of etiologic agents.


【MATERIALS】

- | | | | |
|--|--------------|----------|------------------|
| Materials provided | | | |
| • Test Cassettes | • Droppers | • Buffer | • Package Insert |
| Materials required but not provided | | | |
| • Specimen Collection Containers | • Centrifuge | • Timer | |
| • Lancets (for fingerstick whole blood only) | | | |
| • Heparinized Capillary Tubes and Dispensing Bulb (for fingerstick whole blood only) | | | |

【DIRECTIONS FOR USE】

Allow the test, specimen and buffer controls to reach room temperature (15-30 °C) prior to testing.

- Bring the pouch to room temperature before opening it. Remove the test cassette from the sealed pouch and use it within one hour.
- Place the cassette on a clean and level surface.
For **Serum or Plasma** specimen:
 - Hold the dropper vertically and transfer **2 drops of serum or plasma** (approximately 50 μ L) to the specimen area, then **add 1 drop of buffer** (approximately 40 μ L), and start the timer. See illustration below.For **Venipuncture Whole Blood** specimen:
 - Hold the dropper vertically and transfer **3 drops of whole blood (approximately 75 μ L)** to the specimen area, then **add 1 drop of buffer (approximately 40 μ L)**, and start the timer. See illustration below.For **Fingerstick Whole Blood** specimen:
 - To use a capillary tube: Fill the capillary tube and transfer **approximately 75 μ L of fingerstick whole blood specimen** to the specimen well of test cassette, then **add 1 drop of buffer** (approximately 40 μ L) and start the timer. See illustration below.
 - To use hanging drops: Allow **3 hanging drops of fingerstick whole blood specimen** (approximately 75 μ L) to fall into the specimen well of test cassette, then **add 1 drop of buffer** (approximately 40 μ L) and start the timer. See illustration below.
- Wait for the colored line(s) to appear. **Read results at 10 minutes.** Do not interpret the result after 20 minutes.

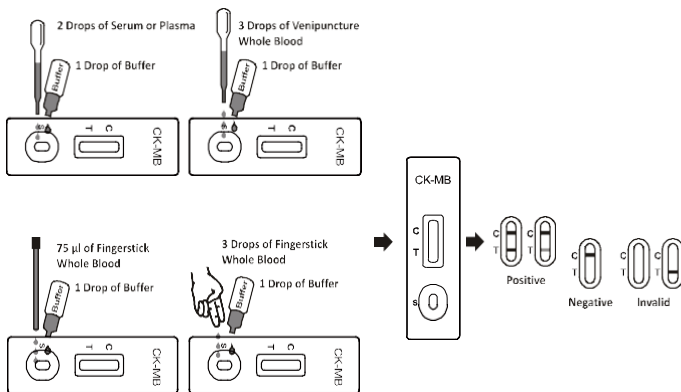

【INTERPRETATION OF RESULTS】

(Please refer to the illustration above)

POSITIVE: * A colored line in the control line region (C) and the presence of another colored line in the test line regions indicates a positive result. This indicates that the concentration of CK-MB is above the minimum detection level.

***NOTE:** The intensity of the color in the test line region(s) will vary depending on the concentration of CK-MB present in the specimen. Therefore, any shade of color in the test line regions should be considered positive.

NEGATIVE: One colored line appears in the control line region (C). No line appears in the test line region (T). This indicates that the concentration of CK-MB are below the minimum detection levels.

INVALID: Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

【QUALITY CONTROL】

A procedural control is included in the test. A colored line appearing in the control line region(C) is considered an internal procedural control. It confirms sufficient specimen volume, adequate membrane wicking and correct procedural technique.

Control standards are not supplied with this kit; however, it is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

【LIMITATIONS】

- The CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma) is for *in vitro* diagnostic use only. This test should be used for the detection of CK-MB in whole blood, serum or plasma specimens only. Neither the quantitative value nor the rate of increase in CK-MB can be determined by this qualitative test.
- The CK-MB Rapid Test Cassette (Whole Blood/Serum/ Plasma) will only indicate the qualitative level of CK-MB in the specimen and should not be used as the sole criteria for the diagnosis of myocardial infarction.
- The CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma) cannot detect less than 5 ng/mL CK-MB in specimens. A negative result at any time does not preclude the possibility of myocardial infarction.
- As with all diagnostic tests, all results must be interpreted together with other clinical information available to the physician.
- Some specimens containing unusually high titers of heterophile antibodies or rheumatoid factor (RF) may affect expected results. Even if the test results are positive, further clinical evaluation should be considered with other clinical information available to the physician.
- There is a slight possibility that some whole blood specimens with very high viscosity or which have been stored for more than 2 days may not run properly on the test cassette. Repeat the test with a serum or plasma specimen from the same patient using a new test cassette.

【PERFORMANCE CHARACTERISTICS】

Sensitivity and Specificity

The CK-MB Rapid Test Cassette (Whole Blood/Serum/ Plasma) has been evaluated with a leading commercial CK-MB ELISA test using clinical specimens. The results show that relative to leading ELISA tests, the CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma) shows >99.9% sensitivity and 99.4% specificity for CK-MB.

CK-MB Rapid Test vs. ELISA

Method		ELISA		Total Results
CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma)	Results	Positive	Negative	
	Positive	62	3	65
	Negative	0	468	468
Total Results		62	471	533

Relative sensitivity: 62/62=>99.9% (95%CI*: 95.3%~100.0%);

Relative specificity: 468/471=99.4% (95%CI*: 98.1%~99.9%);

Accuracy: (62+468)/(62+3+468)=99.4%(95%CI*:98.4%~99.9%) *Confidence Intervals

Precision Intra-Assay

Within-run precision has been determined by using 15 replicates of below five specimens: CK-MB specimen levels at 0 ng/mL, 5 ng/mL, 10 ng/mL, 20 ng/mL and 40 ng/mL. The specimens were correctly identified >99% of the time.

Inter-Assay

Between-run precision has been determined by 3 independent assays on the same five specimens: 0 ng/mL, 5 ng/mL, 10 ng/mL, 20 ng/mL, and 40 ng/mL of CK-MB. Three different lots of the CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma) have been tested using these specimens. The specimens were correctly identified >99% of the time.

Cross-reactivity

The CK-MB Rapid Test Cassette (Whole Blood/Serum/Plasma) has been tested by 3,200 ng/mL CK-MM, 1,700 ng/mL CK-BB, HBsAg, HBsAb, HBeAg, HBeAb, HBcAb, syphilis, anti-HIV, anti-*H.pylori*, MONO, anti-CMV, anti-Rubella and anti-Toxoplasmosis

positive specimens. The results showed no cross-reactivity.

Interfering Substances

The following potentially interfering substances were added to CK-MB negative and positive specimens respectively.

Acetaminophen: 20 mg/dL	Caffeine: 20 mg/dL	Bilirubin: 1,000 mg/dL
Acetylsalicylic Acid: 20 mg/dL	Creatin: 200 mg/dL	Oxalic Acid: 600 mg/dL
Gentisic Acid: 20 mg/dL	Ascorbic Acid: 20 mg/dL	Cholesterol: 800 mg/dL
Hemoglobin: 1,000 mg/dL	Albumin: 10,500 mg/dL	Triglycerides: 1,600 mg/dL

None of the substances at the concentration tested interfered in the assay.

【BIBLIOGRAPHY】

1. Apple FS, Preese LM. Creatine kinase-MB: detection of myocardial infarction and monitoring reperfusion. *J Clin Immunoassay*, 17:24-9, 1994.
2. Lee, T.H., Goldman, L. Serum enzyme assays in the diagnosis of acute myocardial infarction. *Ann Intern Med*, 105:221-233, 1986.
3. Kallner A, Sylven C, Brodin U, et al. Early diagnosis of acute myocardial infarction; a comparison between chemical predictors. *Scand J Clin Lab Invest*, 49:633-9, 1989.

Index of Symbols

	Consult Instructions for Use		Tests per kit		Catalog #
	For <i>in vitro</i> diagnostic use only		Use by		Do not reuse
	Store between 2-30°C		Lot Number		
	Do not use if package is damaged		Manufacturer		

ICT International
10 Fleur de Lage
Sovereign Rd
Johannesburg
South Africa
Tel: +27 73 955 0524
Email: info@ictdiagnostics.co.za

Number: 14601102600
Revision date: 2022-09-21